



1/6

Fig. 1

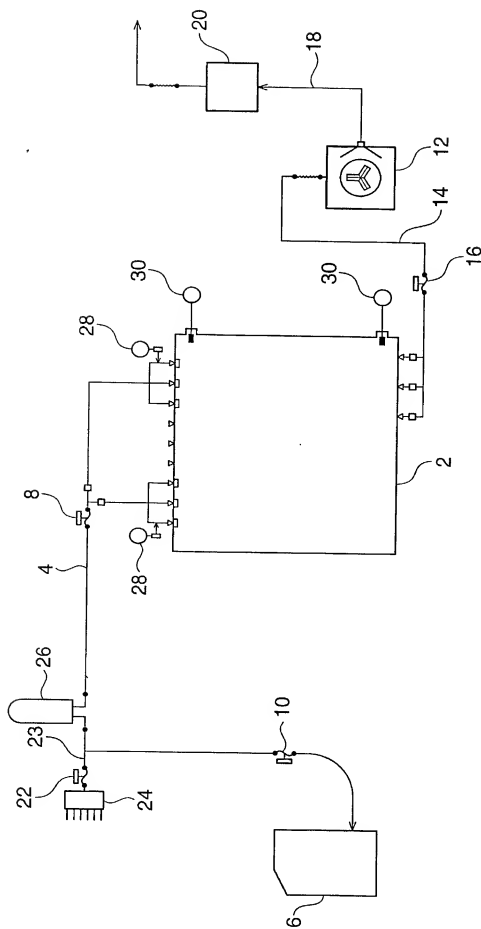

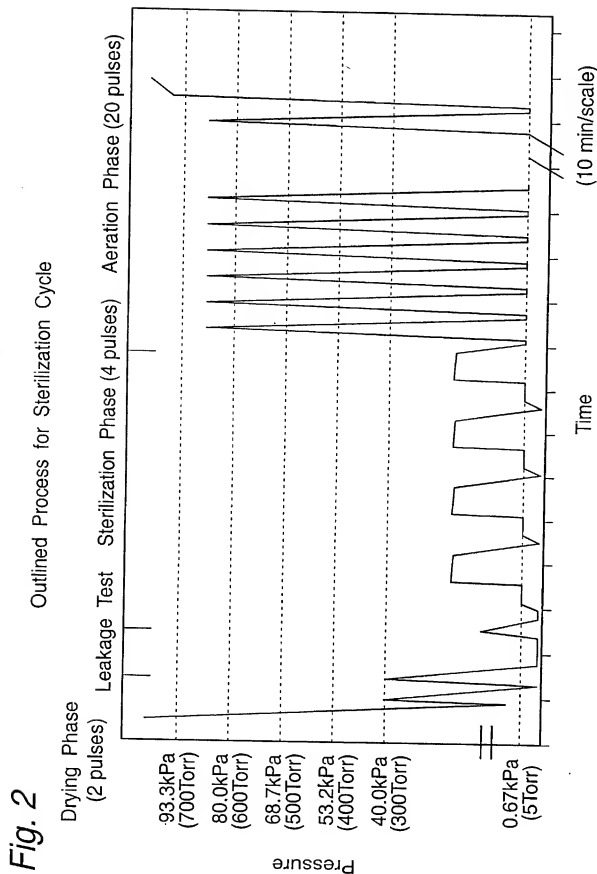

In case where the sterilization cycle comprises a combination of 4 pulses of gaseous hydrogen peroxide treatment and 20 aeration pulses, the sterilization process requires about 3 hours and 20 minutes.

3/6



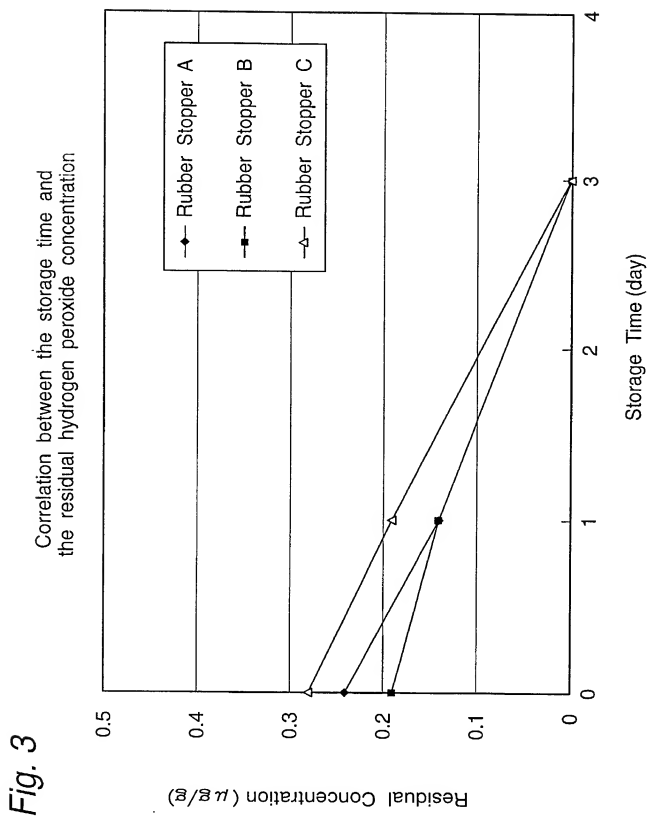


Fig. 4

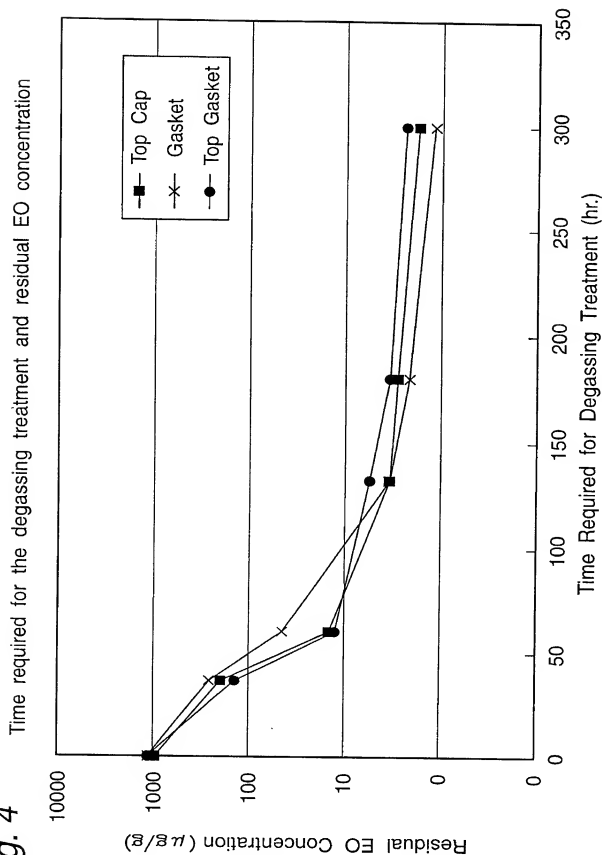

5/6

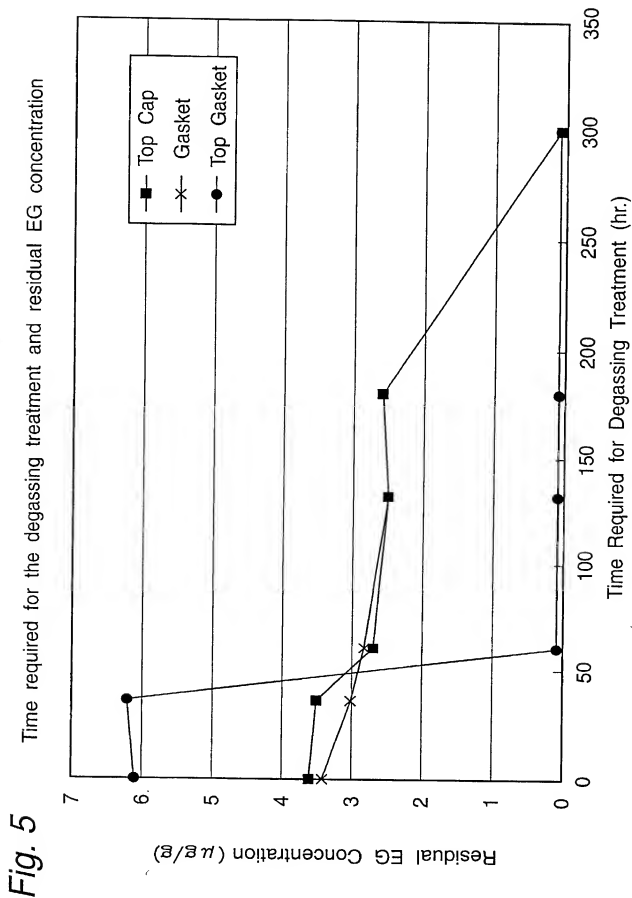

6/6

Fig. 6

